

FIG. 1A.

TOPIC "SEEDED"

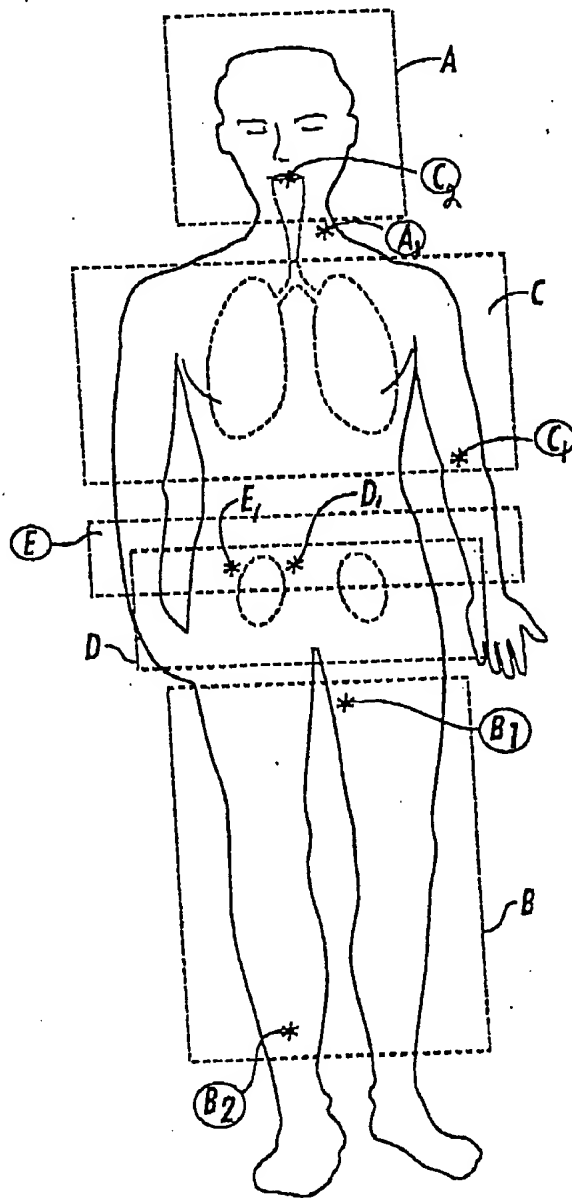


FIG. 1B.

25

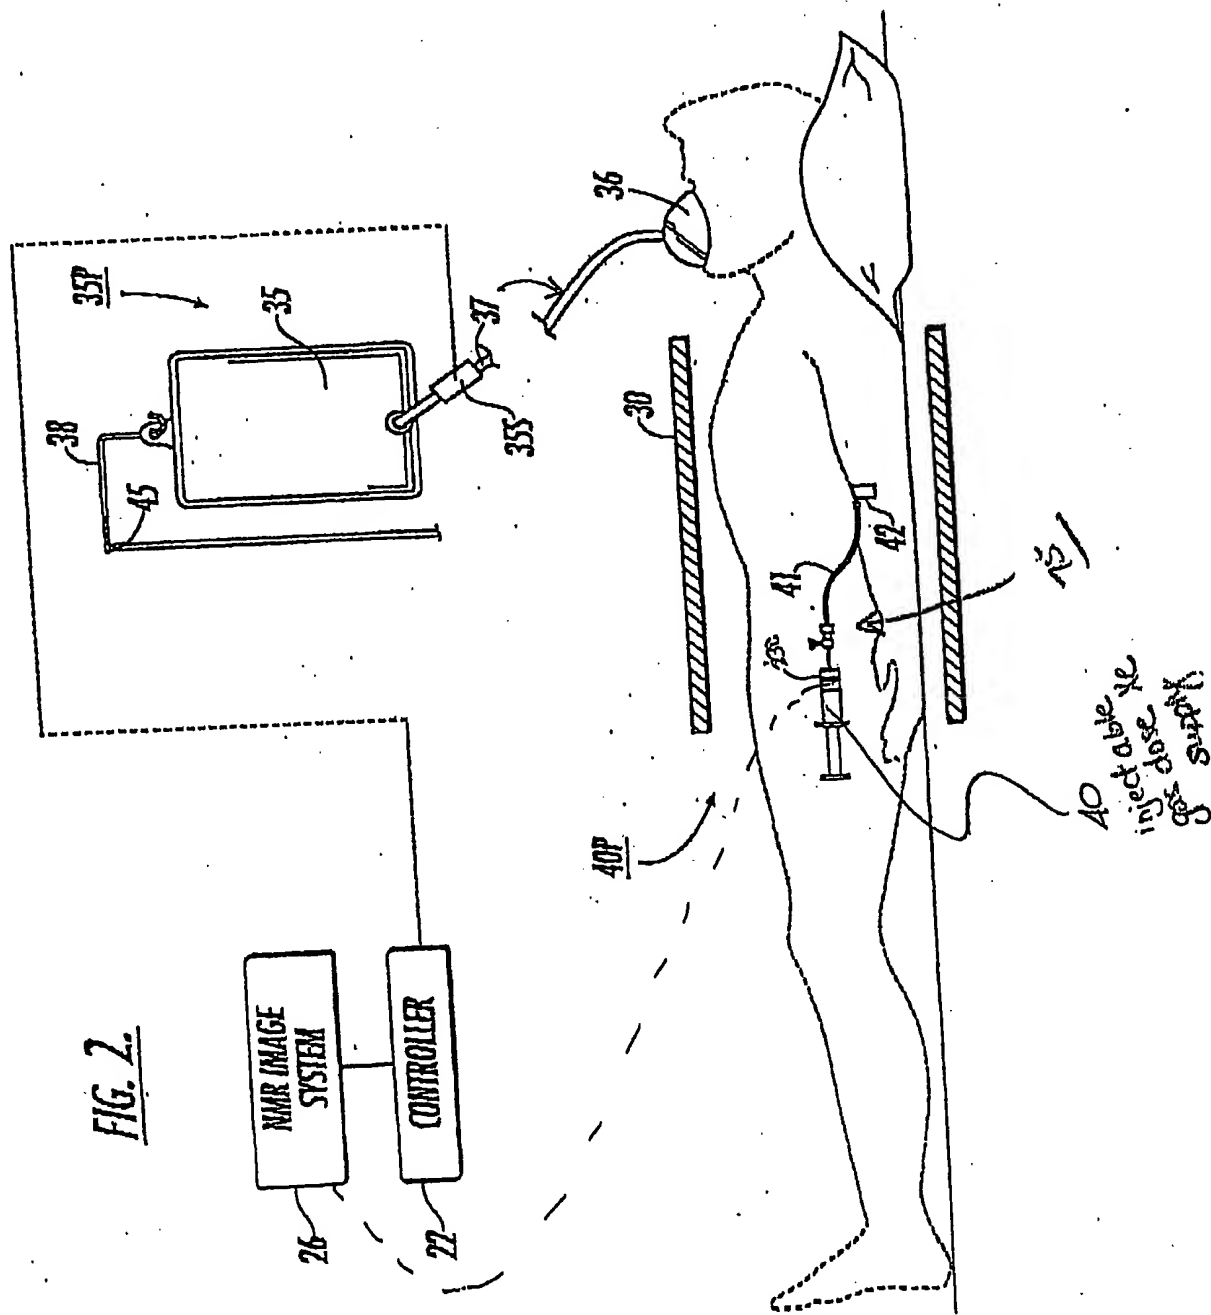


FIG. 2

NMR IMAGE SYSTEM

CONTROLLER

26

27

40P

30

36

35

37

38

45

35P

40
injectable drug
dose supply

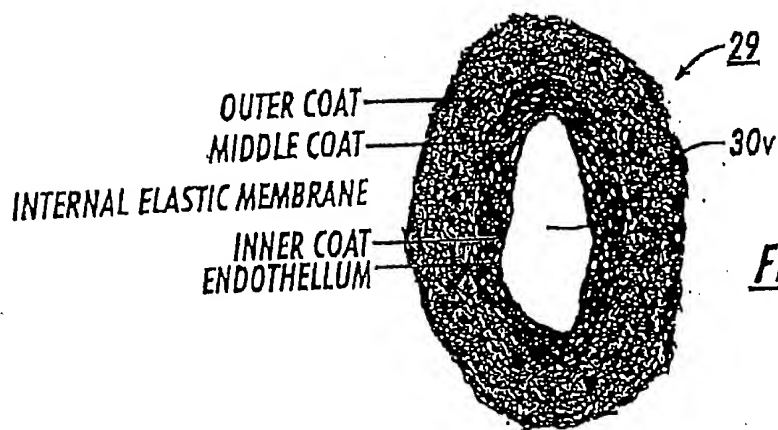


FIG. 3A.

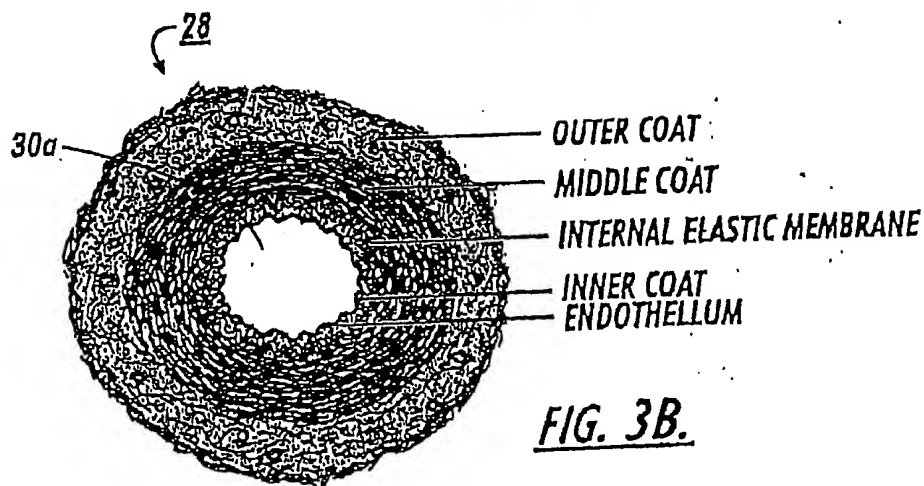


FIG. 3B.

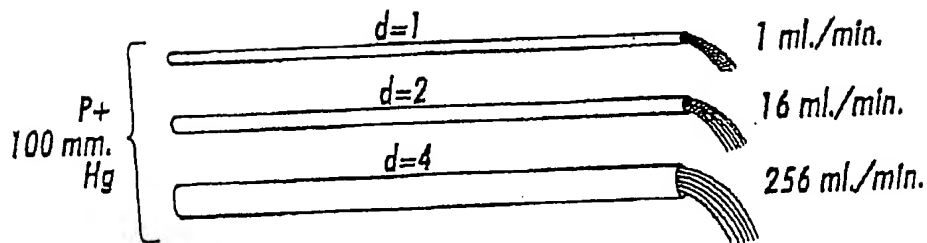
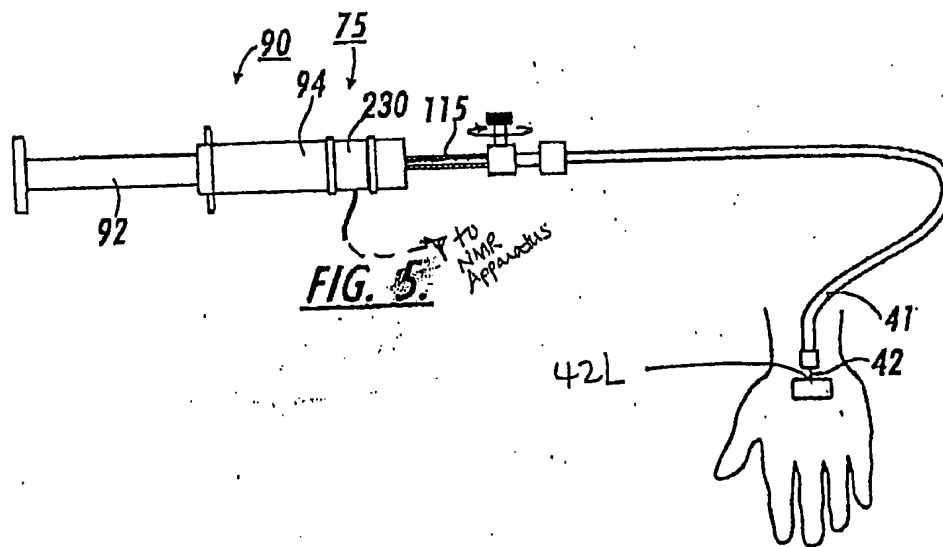
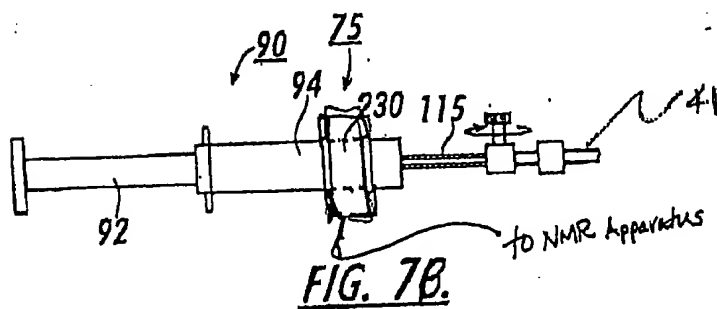
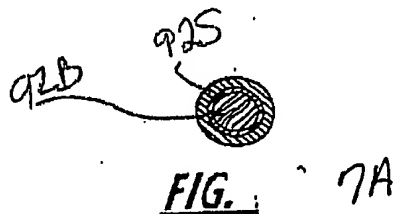
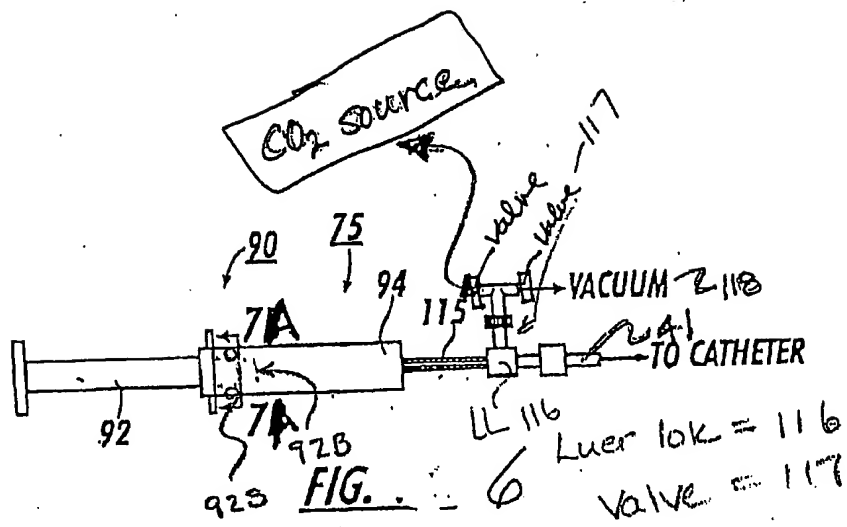
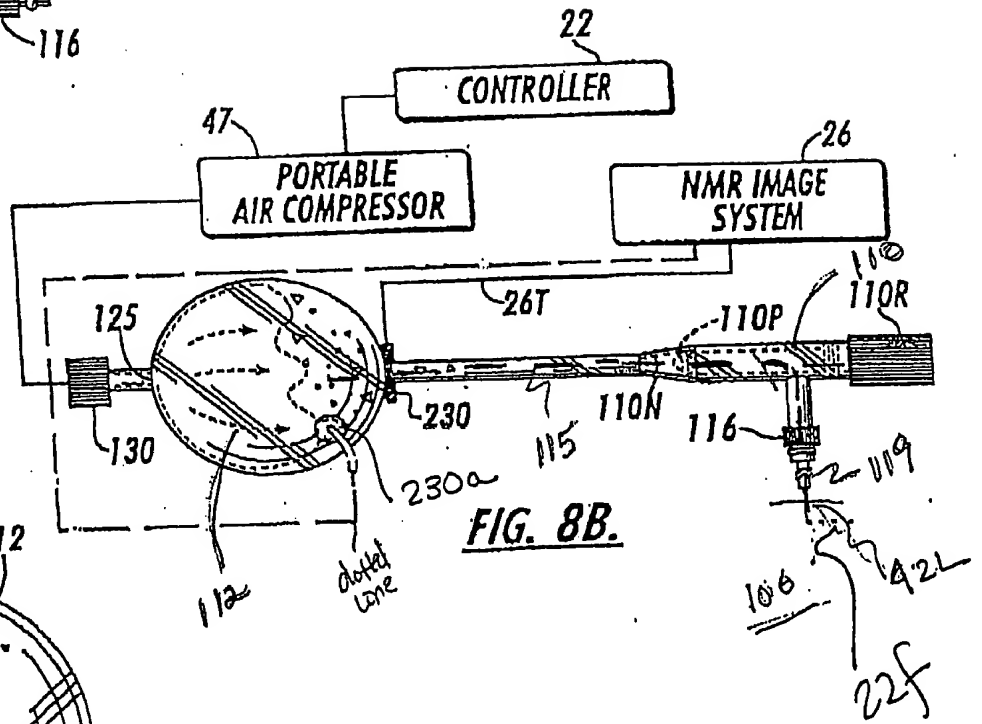
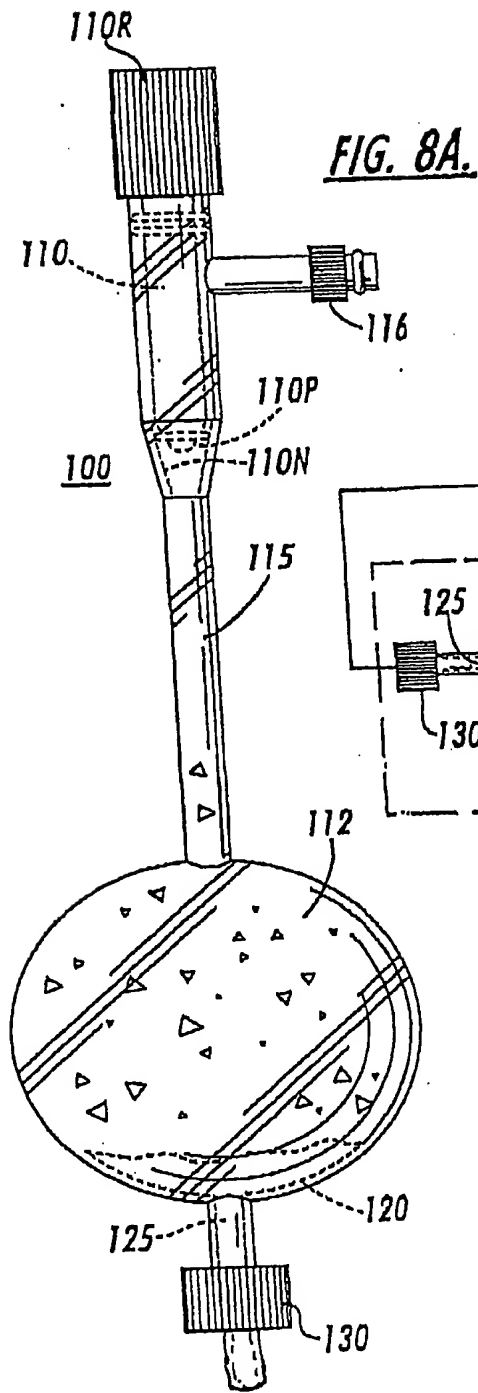


FIG. 4







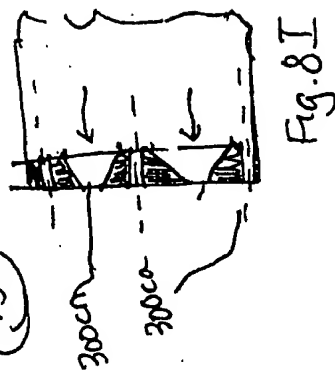
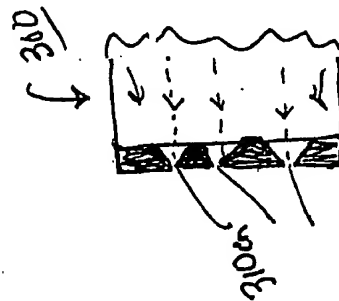
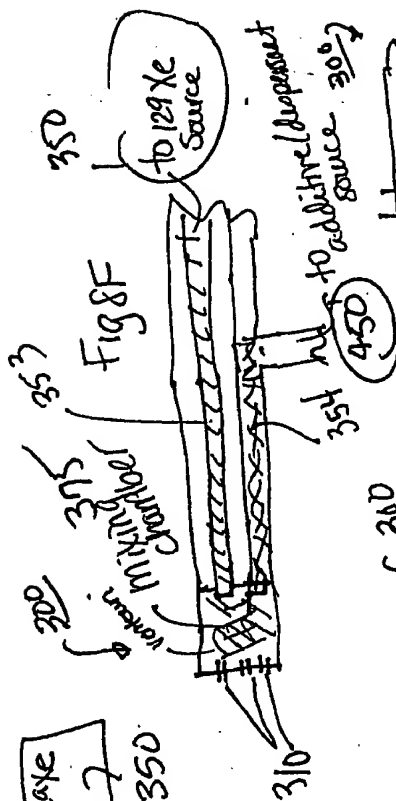
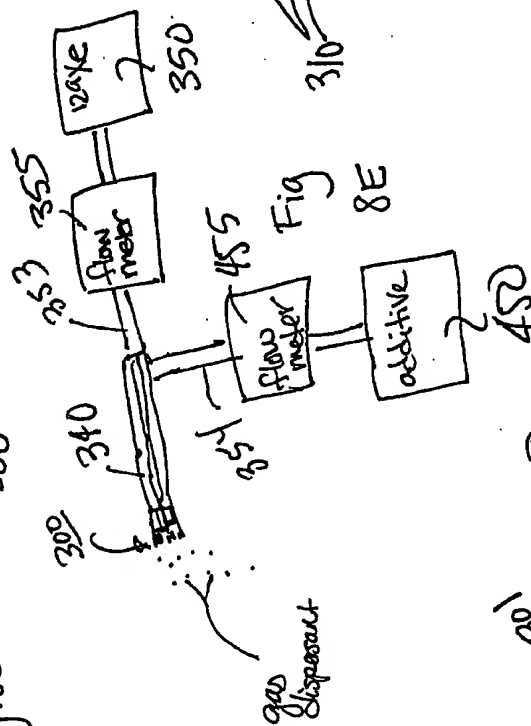
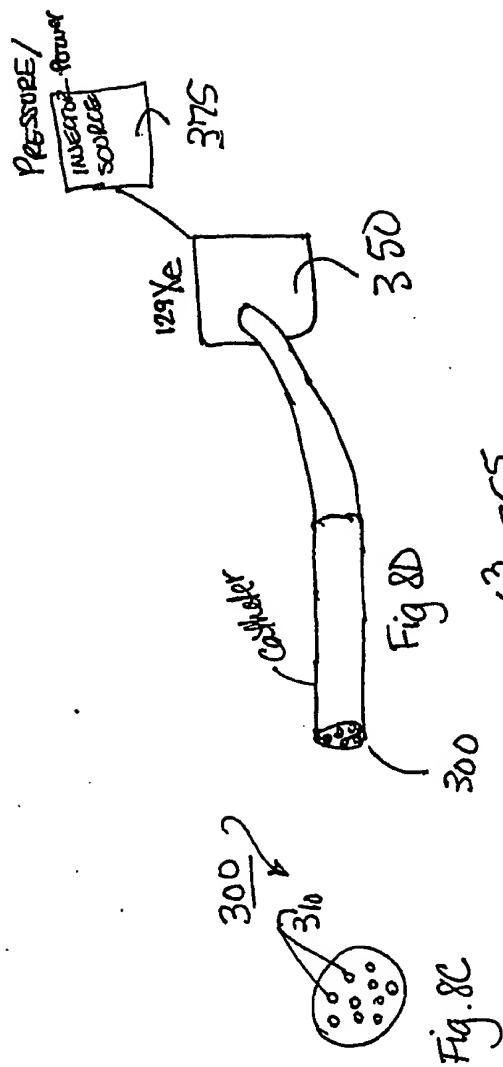


Fig 8.5
mixing chamber
convergent nozzles

Fig 8G

REF ID: A66060

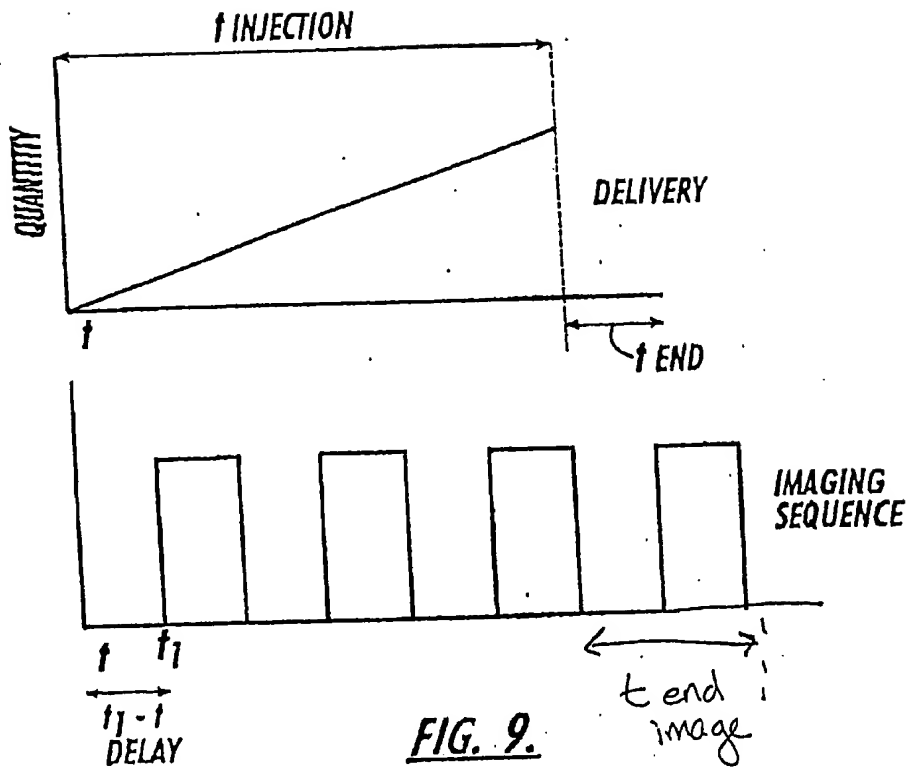


FIG. 9.

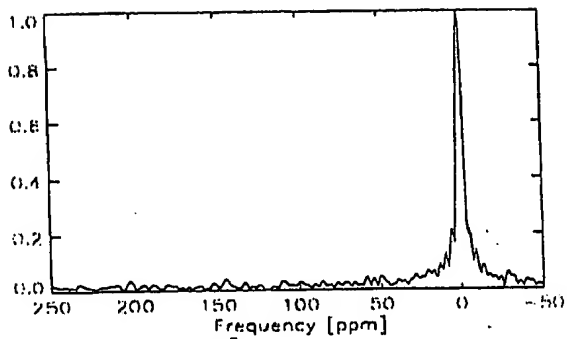


Fig 10A

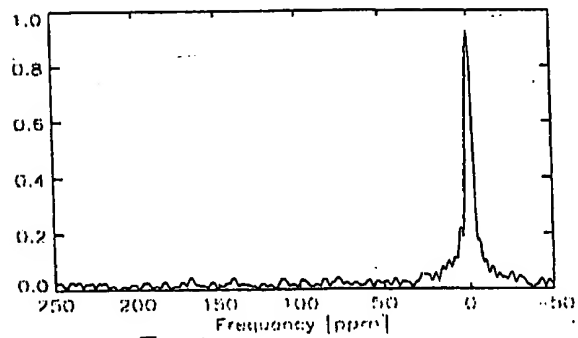


Fig 10B

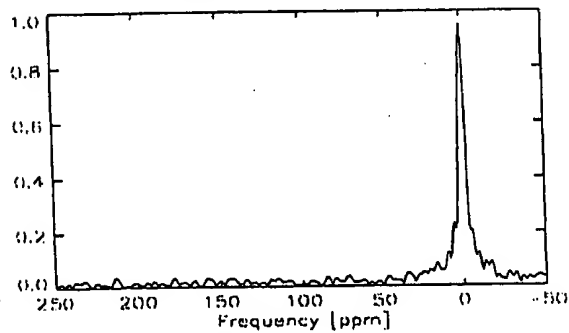


Fig 10C

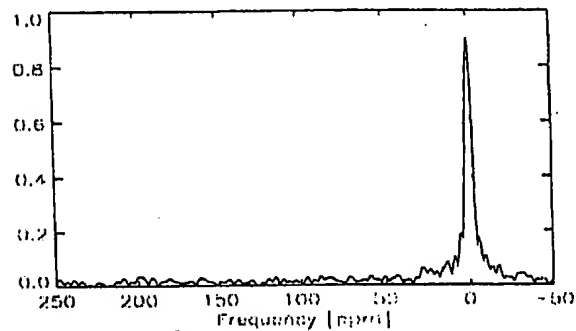


Fig 10D

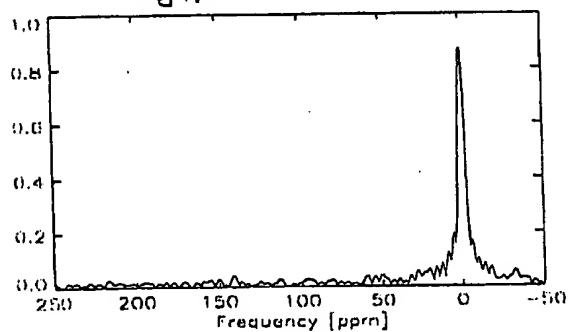


Figure 10E

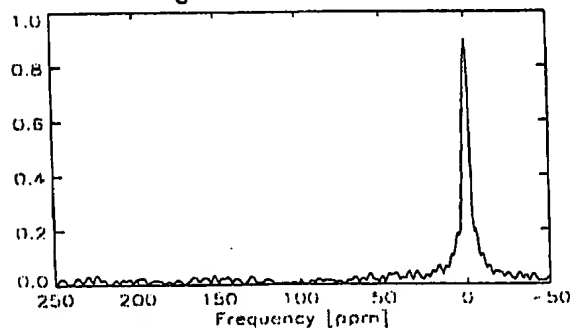


Fig 10F

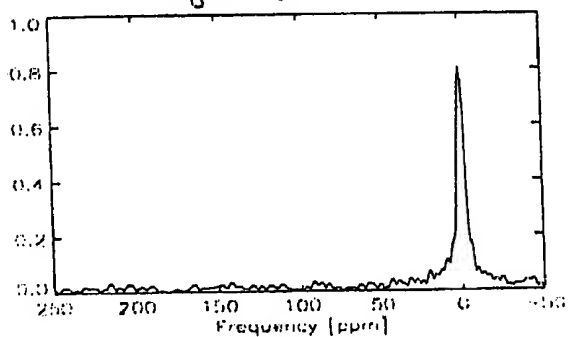


Fig 10G

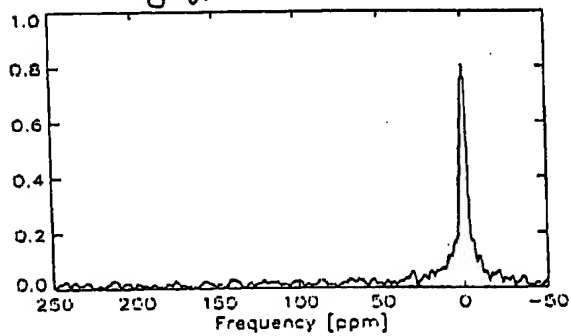


Fig 10H

20250606

Fig 10 I

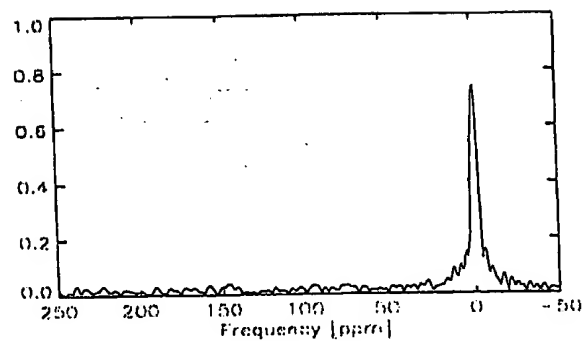


Fig 10J

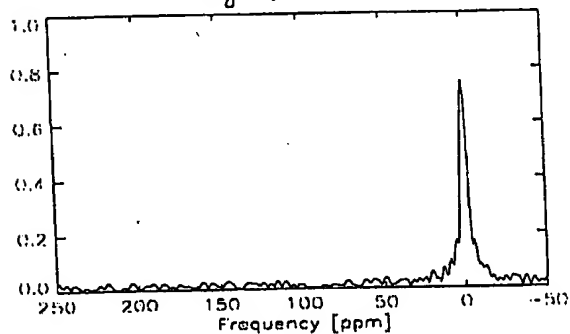


Fig 10 K

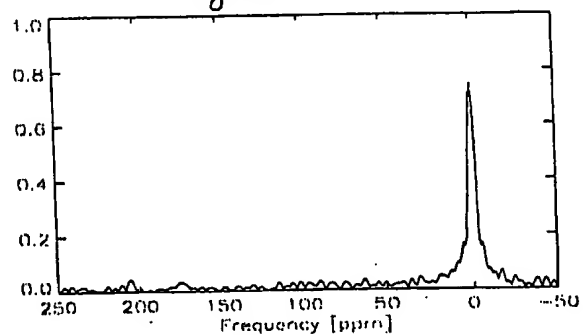


Fig 10 L

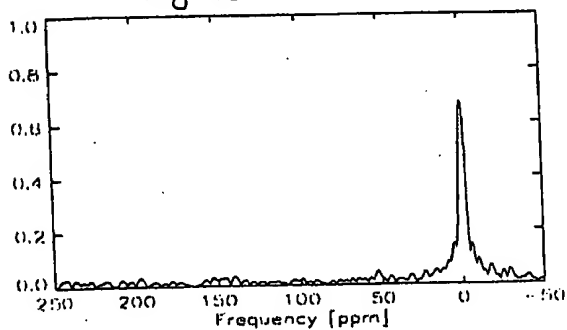


Fig 10 M

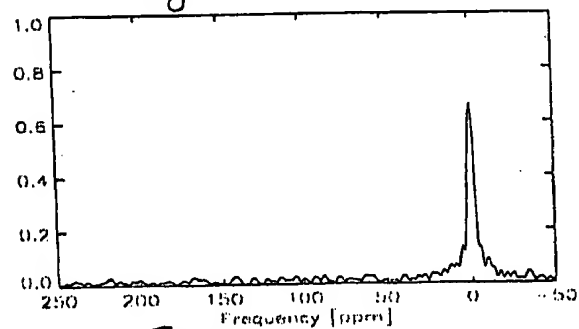


Fig 10 N

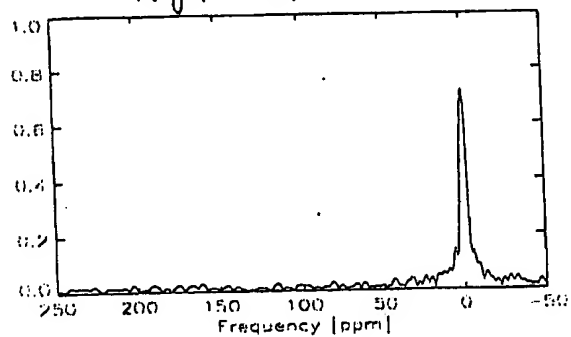


Fig 1B 0

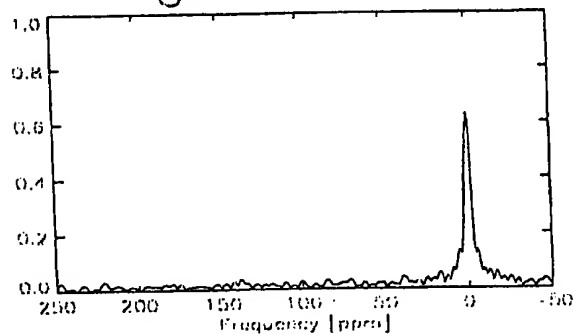


Fig 10 p

FOOTED 69E0660

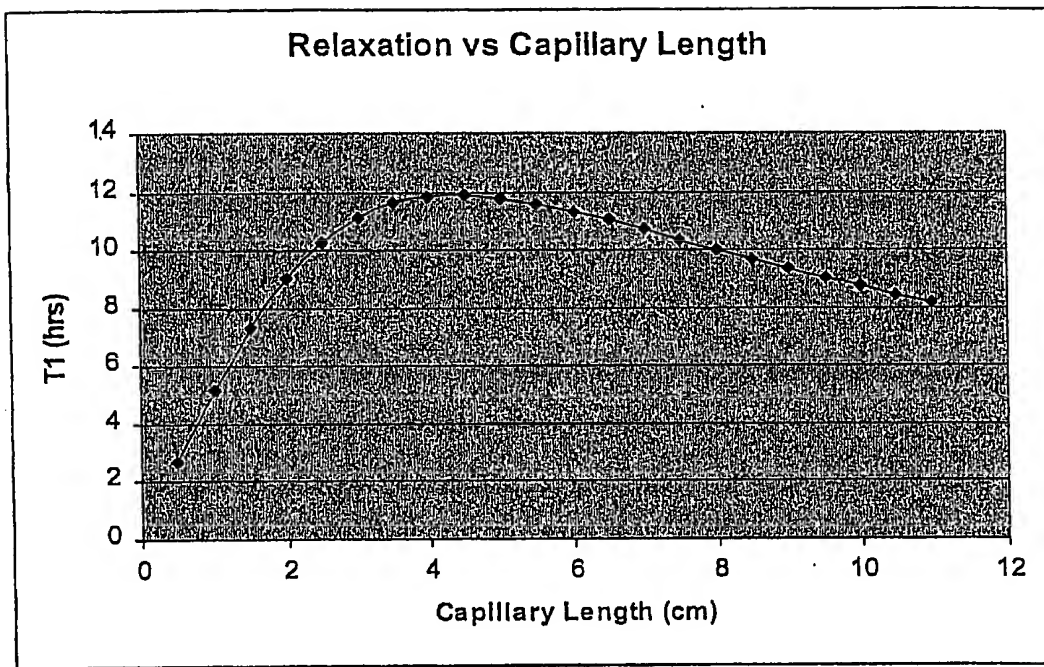


Fig 11